

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problems Mailbox.**

PCT

WORLD INTELLECTUAL PROPERTY ORGANIZATION  
International Bureau




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<p>(51) International Patent Classification 6: G01N 21/76</p>	<p>A2</p>	<p>(11) International Publication Number: WO 95/07457 (43) International Publication Date: 16 March 1995 (16.03.95)</p>
<p>(21) International Application Number: PCT/GB94/01706 (22) International Filing Date: 3 August 1994 (03.08.94) (30) Priority Data: 9318495.0 7 September 1993 (07.09.93) GB (71) Applicant (for all designated States except US): BIOTRACE LIMITED (GB/GB); The Science Park, Bridgend, Mid Glamorgan CF31 3NA (GB). (72) Inventors; and (75) Inventors/Applicants (for US only): JOHNSON, Ian, Roy (GB/GB); Windsford, 25 Heol St. Bridget, St. Bridges Major, Mid Glamorgan CF31 0SL (GB). GOODFIELD, Clive (GB/GB); 69 Cood Isaf Road, Maesycoed, Pontypidd, Mid Glamorgan CF37 1EN (GB). (74) Agent: GIBSON, Stewart, Harry; Urquhart-Dykes &amp; Lord, Three Trinity Court, 21-27 Newport Road, Cardiff CF2 1AA (GB).</p>		<p>(81) Designated States: AU, CA, FI, JP, US, European patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).  Published Without international search report and to be republished upon receipt of that report.</p>

(54) Title: BIO-LUMINESCENCE MONITORING APPARATUS AND METHOD

(57) Abstract

A monitoring instrument (or luminometer) comprises a casing (10) having a section (14) which can be pivoted between one position generally flush with a top face of the casing, and a second position which is generally vertical. The pivoted section (14) includes an elongate sample chamber (15) to receive a sample. The instrument has a light detector arrangement for sensing light emitted from a sample inserted into the sample chamber, to provide a measure of the light emitted in a predetermined time period. The instrument is used for monitoring bio-luminescent light emission, in which a swab, pre-moistened with breakage reagent, is wiped over a surface to be tested, then contacted with enzyme solution so that light will be emitted from the swab sample if it has picked up cells: the swab is then inserted into a transparent tube which is placed in the sample chamber (15).

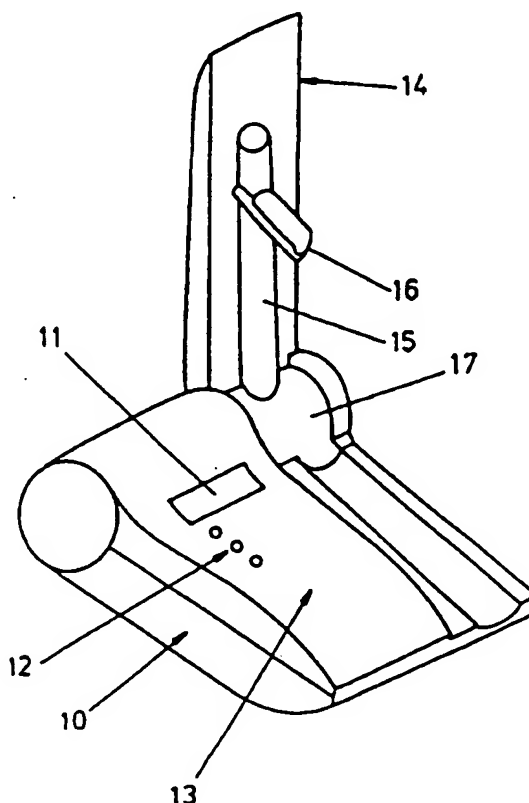

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	GB	United Kingdom	MR	Mauritania
AU	Australia	GE	Georgia	MW	Malawi
BS	Barbados	GN	Guinea	NE	Niger
BE	Belgium	GR	Greece	NL	Netherlands
BF	Burkina Faso	HU	Hungary	NO	Norway
BG	Bulgaria	IE	Ireland	NZ	New Zealand
BJ	Benin	IT	Italy	PL	Poland
BR	Brazil	JP	Japan	PT	Portugal
BY	Belarus	KE	Kenya	RO	Romania
CA	Canada	KG	Kyrgyzstan	RU	Russian Federation
CF	Central African Republic	KP	Democratic People's Republic of Korea	SD	Sudan
CG	Congo	KR	Republic of Korea	SE	Sweden
CH	Switzerland	KZ	Kazakhstan	SI	Slovenia
CI	Côte d'Ivoire	LI	Liechtenstein	SK	Slovakia
CM	Cameroon	LR	Liberia	SN	Senegal
CN	China	LU	Luxembourg	TD	Chad
CS	Czechoslovakia	LV	Latvia	TG	Togo
CZ	Czech Republic	MC	Monaco	TJ	Tajikistan
DE	Germany	MD	Republic of Moldova	TT	Trinidad and Tobago
DK	Denmark	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	US	United States of America
FI	Finland	MN	Mongolia	UZ	Uzbekistan
FR	France			VN	Viet Nam
GA	Gabon				

Bio-luminescence Monitoring Apparatus and Method

This invention relates to an apparatus and method for monitoring bio-luminescent light emission, particularly but not solely for use in hygiene monitoring.

It is known to test for micro-organisms or other cellular material by taking a sample and releasing adenosine triphosphate (ATP) contained within the cells using an appropriate reagent together with the enzyme luciferase in order to cause the emission of light. The light output is related to the concentration of ATP in the sample and hence the contamination present.

Hitherto, a typical testing procedure has involved wiping a pre-moistened swab over a surface to be tested, contacting the swab with a breakage reagent to transfer bacteria or cells from the swab to that reagent and thereby releasing cellular ATP, then transferring the extract to a cuvette containing a liquid of the enzyme luciferase, such that light is now emitted from the liquid in the cuvette. The cuvette is now placed into a light-tight chamber of a monitoring instrument, or luminometer, which measures the light output over a predetermined period of time (typically 10 seconds): this measured light is a measure of the quantity of cells picked up on the swab. The procedure depends upon transferring cells from the surface to the swab and then to the breakage reagent, but in practice this is inefficient because only a proportion of the cells will be transferred.

In accordance with this invention, there is provided a method of testing, comprising wiping a swab, pre-moistened with breakage reagent, over a surface to be tested, contacting said swab with enzyme solution such that if the swab sample has picked up cells, light is now emitted, then measuring the light output directly from the swab.

This method avoids inaccuracies associated with transfer and dilution losses of hitherto known methods using ATP extraction.

The swab is moistened with breakage reagent before it is wiped over the surface to be tested. Preferably a number

of swabs are pre-moistened in this manner, then enclosed in protective tubes until required for use. After wiping over the surface to be tested, preferably the swab is dipped into the enzyme solution for a pre-determined time period (e.g. 60  
5 seconds), then returned to its protective tube. This tube is preferably transparent so that it can then be introduced into the monitor to measure the light now being emitted from the swab owing to the release of ATP from the cells picked up on the swab from the surface being tested. We have found that  
10 polyethylene often emits a low level of light, by autofluorescence: we have found that polypropylene does not exhibit autofluorescence and is therefore a suitable material for the protective tubes for the swabs used in this method.

Also in accordance with this invention, there is  
15 provided a monitoring instrument (luminometer) comprising a casing having a section which can be pivoted between one position generally flush with a top face of said casing and a second position which is generally vertical, said section including an elongate sample chamber to receive a sample, the  
20 instrument further including a light detector arrangement for sensing light emitted from a sample in said chamber and providing a measure of the light emitted in a predetermined time period.

This instrument is able to receive an elongate sample  
25 for measurement of its light output: for this purpose the pivoted section is moved to its generally vertical position. However, when not required for use, this pivoted section can be pivoted to its position generally flush with the top face of the instrument casing.

30 The luminometer is thus able to receive a swab when returned to its protective tube, or sample tube. Preferably a light tight cap is provided for the open top end of the elongate sample chamber, and this cap is slidable into a position in which it detents: in being slid into this  
35 position, the cap bears on the top of the sample tube within the sample chamber, to depress the sample tube and correspondingly displace a member on which the sample tube rests; this member now bears against a shutter to pivot the

latter from an opening to the light detector.

Embodiments of this invention will now be described by way of example only and with reference to the accompany drawings in which:

5       FIGURE 1 is a perspective view of a monitoring instrument or luminometer in accordance with this invention, shown with its sample chamber section pivoted to a closed position;

FIGURE 2 is a similar view of the instrument, shown 10 with its sample chamber section pivoted to an in-use position;

FIGURE 3 is an enlarged vertical section across the instrument adjacent its rear edge;

FIGURE 4 is a section on the line IV-IV of Figure 3; and

15       FIGURE 5 shows a swab, swab protective tube and an enzyme containing tube used with the luminometer in a kit.

Referring to Figures 1 and 2, there is shown a luminometer the housing or casing 10 of which is of generally rectangular, flat form arranged for the monitor to rest flat 20 on a table, bench or the like. The top face of the casing 10 has a window 11 through which a numerical display is presented, a number of translucent windows 12 through which indicator lights (LED's) are visible when energised, and a touch-sensitive panel 13 to operate a "start" switch of the 25 instrument. The luminometer further comprises an elongate section 14 extending from front-to-rear of the casing 10 along its right hand side, this elongate section 14 being pivoted to the casing at the rear of the latter. Normally the section 14 is in a closed position in which it lies flush with the top 30 surface of the casing, as shown in Figure 1, but the section 14 can be pivoted to an upright position as shown in Figure 2.

The pivoted section 14 is formed on its underside with an elongate, tubular chamber 15 which has an open top normally closed by a light-tight cap 16. At its bottom end, the tubular 35 chamber 15 merges into a larger-diameter cylinder 17 which is mounted for pivoting about its axis, to provide the pivotal movement of the section 14. As shown in Figure 3, the opposite ends of cylinder 17 are journaled in fixed annular flanges of

the casing 10: one end 18 of the cylinder 17 is closed, whilst its other end is open but journaled to a fixed circular wall 19 having an integral tube 21 which extends across the width of the casing 10 adjacent its rear edge and bottom wall: the tube 21 houses a photomultiplier P the sensor face of which lies just behind an end 20 of tube 21 which projects into the cylinder 17. A shutter 22 is pivoted to the fixed wall 19 and normally lies across the end 20 of tube 21 to prevent light reaching the photomultiplier P. Alternative forms of light detector may be used instead of the photomultiplier, e.g. an avalanche photodiode or junction light detecting device.

The cylinder 17 has a member 23 slidably mounted in it, as shown in Figure 3. Member 23 is a transparent tube, closed at its lower end, and having a skirt 24 depending from its top and extending around it. The member 23 is biased upwards by a compression spring (not shown). When the member 23 is depressed against the bias of its spring, the lower edge of the skirt 24 bears against a projecting pin 26 on the shutter 22 to pivot the latter about point 25 to its open position (Figure 4).

The luminometer casing 10 houses a pack of rechargeable batteries against its bottom wall and above this a main circuit board is mounted. The liquid crystal display is mounted on a further circuit board above the main circuit board.

In use to measure the light output of a sample, the sample swab is inserted into an elongate plastics sample tube 28 as will be described below. This sample tube 28 is then inserted into the elongate chamber 15 of the section 14, so that its lower end is received by the tubular slidable member 23 in the cylinder 17. Then the cap 16 is pivoted up to an in-line position over the top of the elongate chamber 15, and is then pressed down to a position in which it detents: during this movement, the cap 16 bears on the top of the sample tube 28 to press the latter downwards, and in so doing depressing the tubular member 23 against its spring bias, and in turn opening the shutter 22. In its detented position, the cap 16 closes the top of the elongate chamber 15 in light-tight manner, and also operates a switch, preferably a micro-switch

to enable the electronic circuit of the monitor.

Now the user starts the luminometer, using the touch-sensitive panel 13, and the light output received by the photomultiplier, in a predetermined period of time, is measured  
5 and displayed as a numerical count. The luminometer will not start unless it is enabled by closure of the switch by the cap.

In order to prepare a sample, a swab as shown in Figure 5 is used: the swab 30 is in the form of an absorbent bud on the end of an elongate stalk 31. The swab 30 has been pre-  
10 moistened by dipping into an appropriate swabbing solution (ATP breakage reagent), and then stored in an elongate tube. The swab 30 is wiped back-and-forth over e.g. a work-surface to be tested, at the same time turning the stalk 3 so that the whole periphery of the swab 30 will come into contact with the work-  
15 surface. During the swabbing, the ATP is released from cellular material picked up from the surface being wiped. The swab is then dipped into a small tube 32 containing enzyme solution so that light is emitted. The swab is then put back into the sample tube 28, which is then introduced into the  
20 instrument to measure the light output.

Preferably the luminometer is used in a kit which comprises a carrying case for housing the instrument, a plurality of swabs in their protective tubes 28, a plurality of enzyme-containing tubes 32 and a stand for holding the  
25 latter tubes. The swab stalk has a plug at its upper end to seal into the top of the tube 28, and the enzyme-containing tube 28 is formed with an integral plug. In use of this kit, the swabs may be pre-moistened and stored in their protective tubes and the tubes filled with enzyme, all at a central  
30 laboratory, to enable easy use of the kit in the field, and has the benefit of being "food factory safe" as the kit does not contain any glass or wooden parts which would be hazardous in such environments.





Claims

- 1) A monitoring instrument, comprising a casing having a section which can be pivoted between one position generally flush with a top face of said casing and a second position  
5 which is generally vertical, said section including an elongate sample chamber to receive a sample, the instrument further including a light detector arrangement for sensing light emitted from a sample in said chamber and providing a measure of the light emitted in a predetermined time period.
- 10 2) A monitoring instrument as claimed in claim 1, further comprising a light tight closure for the open top end of said elongate sample chamber.
- 3) A monitoring instrument as claimed in claim 2, in which said closure is slidable into a position closing said open top  
15 end of the sample chamber, for depressing a sample tube disposed within said chamber, a member being provided on which said sample tube sits, said member being depressed upon depression of said sample tube to cause a shutter of the light detector arrangement to be opened.
- 20 4) A method of testing, comprising wiping a swab, pre-moisted with breakage reagent, over a surface to be tested, contacting said swab with enzyme solution such that if the swab sample has picked up cells, light is now emitted, then measuring the light output directly from the swab.
- 25 5) A method as claimed in claim 4, in which the pre-moistened swab is enclosed and stored in a protective tube prior to use.
- 6) A method as claimed in claim 5, in which the swab is dipped into the enzyme solution for a predetermined time and  
30 then returned to its protective tube.
- 7) A method as claimed in claim 6, in which said

protective tube is transparent and is next introduced into a monitor to measure the light emitted from the swab sample.

-1/3-

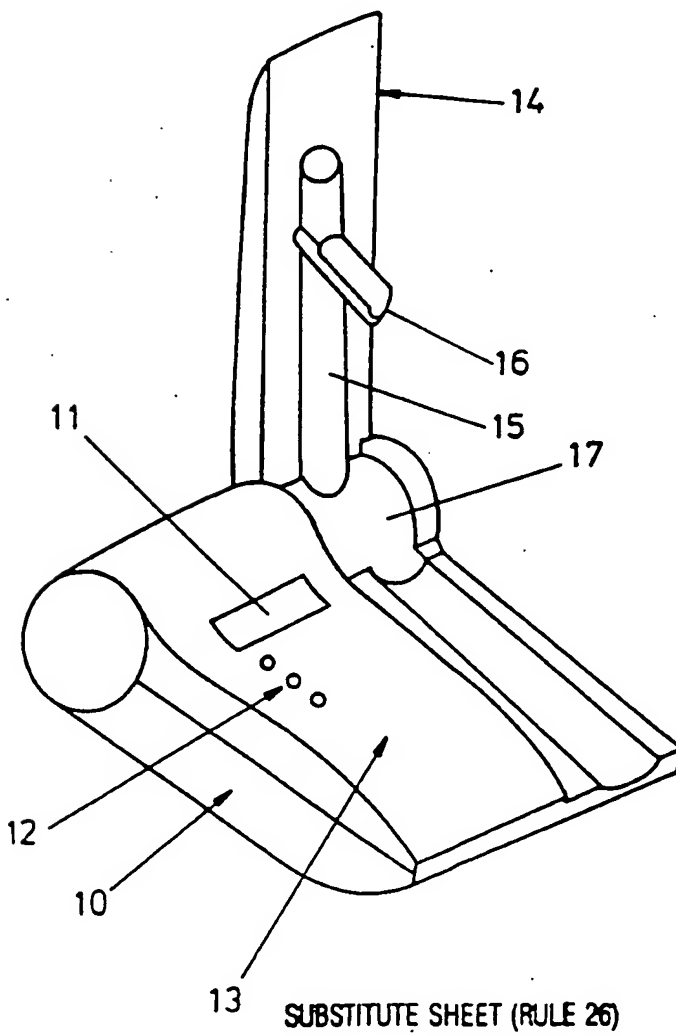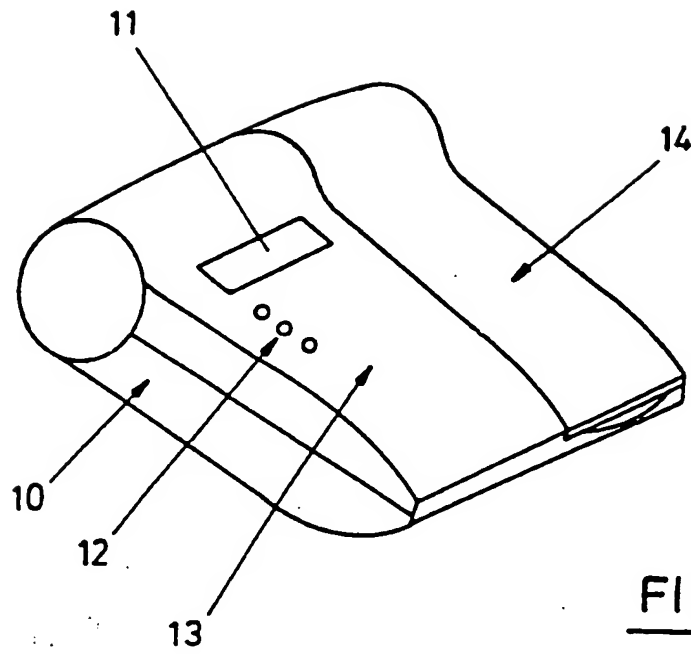

-2/3-

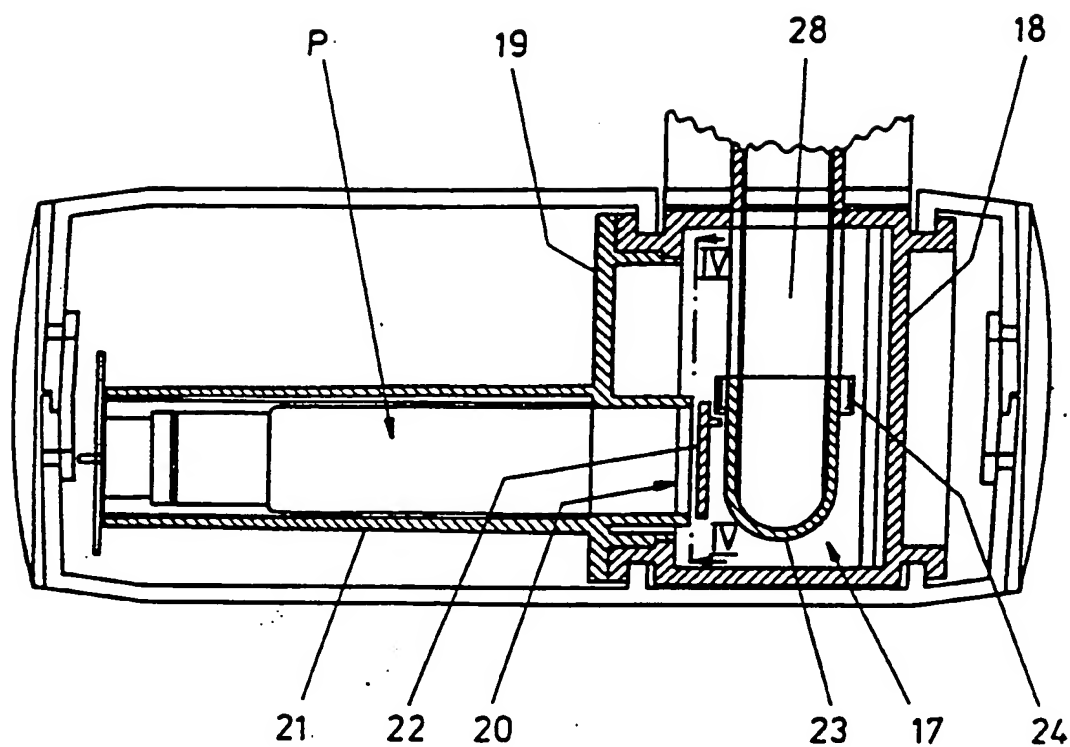


FIG. 3

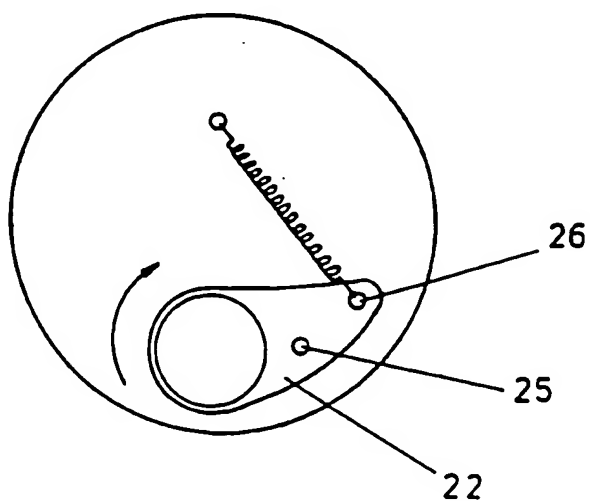
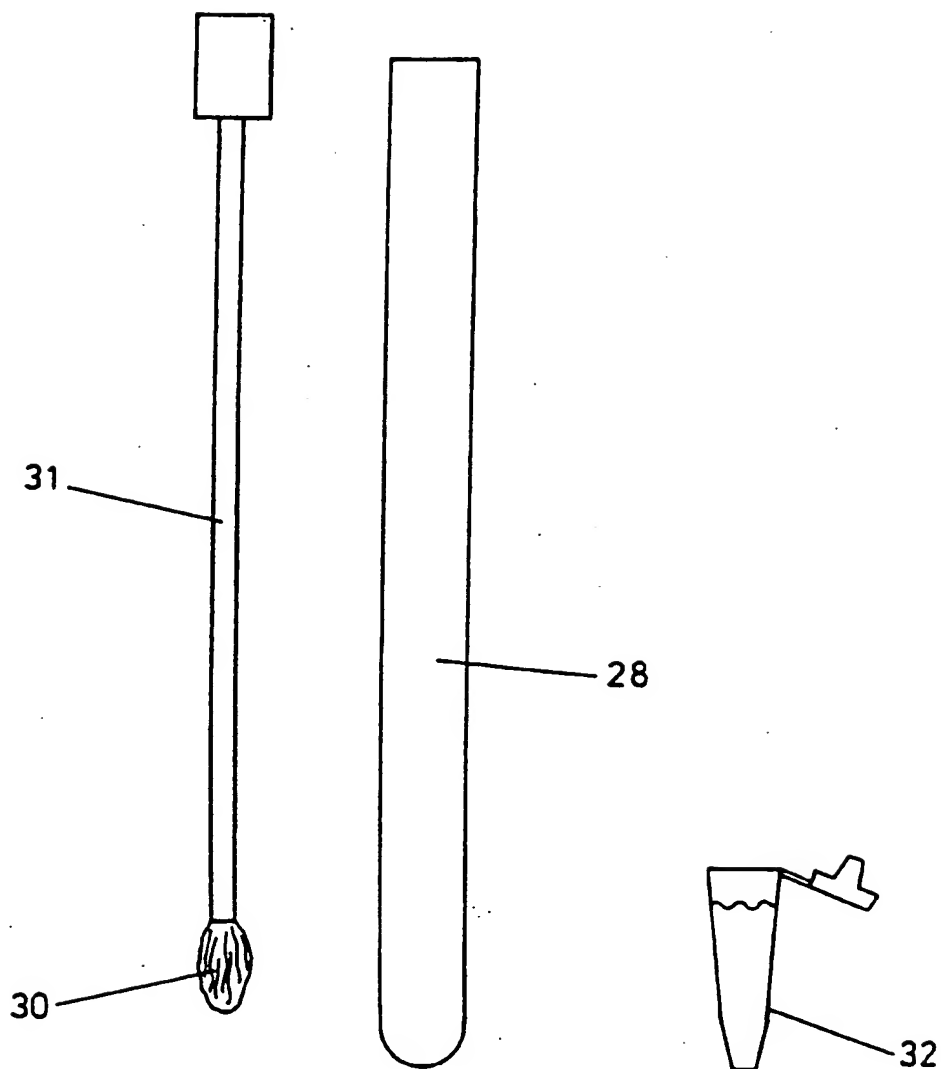


FIG. 4

SUBSTITUTE SHEET (RULE 26)

- 3 / 3 -

FIG. 5